

abia fT3




REF DK.034.01.3

IVD



Note: Changes highlighted ★

abia

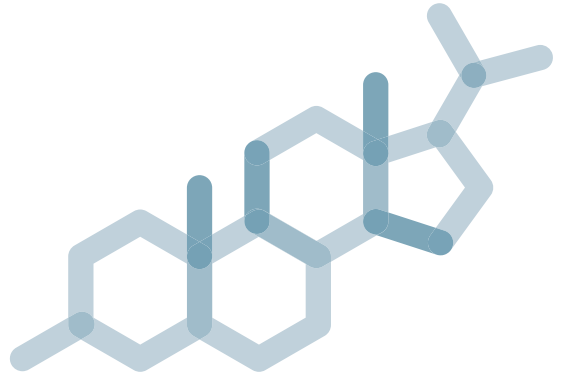

Intended use

Abia fT3 enzyme immunoassay for the quantitative determination of free triiodothyronine (fT3) concentration in human serum.

The assay is intended for aid in the assessment of thyroid status and diagnosis of thyroid disease. For professional use only.

Clinical value

Triiodothyronine (T3), the principal thyroid hormone, circulates in blood almost completely bound to carrier proteins.

The main carriers are thyroxine-binding globulin (TBG), pre-albumin and albumin. However, only the free (unbound) portion of triiodothyronine is responsible for the biological action. Total T3 consists of both the bound and unbound fractions. Further, the concentrations of the carrier proteins are altered in many clinical conditions, such as pregnancy.

In normal thyroid function as the concentrations of the carrier proteins alters, the total triiodothyronine level changes so that the free triiodothyronine concentration remains constant. Diseases affecting thyroid function may present a wide array of confusing symptoms.

Measurement of free T3 by immunoassay is the reliable and convenient test available to determine the presence of thyroid disorders in patients. Increased levels of fT3 have been found in hyperthyroidism. Low levels of fT3 have been associated with hypothyroidism.

Principle of the test

Abia fT3 is a one-step immunoassay, based on the principle of the competitive method.

Free triiodothyronine present in the sample and the labeled enzyme-triiodothyronine in the conjugate compete for binding to the capture antibody on the anti-T3 coated microplate. The enzyme activity in the antibody-bound fraction is inversely proportional to the native triiodothyronine concentration.

The unbound components are removed by washing. After addition of the solution containing TMB and hydrogen peroxide, the wells with bound conjugate develop a blue colour which is converted to yellow after the reaction has been stopped with sulphuric acid.

The colour intensity is inversely proportional to the concentration of the native free triiodothyronine in the specimen and can be read at 450 nm.

Kit contents

	S	
T3 Ab coated plate	1	polystyrene plate 12 × breakable 8-well strips coated with monoclonal anti-triiodothyronine Ab
Conjugate	1 × 12 ml	ready to use; HRP-labeled triiodothyronine; transparent or slightly opalescent pink liquid
Calibrator 0	1 × 0.5 ml	human serum not containing ft3; pale yellow liquid
Calibrator 1	1 × 0.5 ml	human serum containing ft3 in concentration approx. 1.5 pg/ml; pale yellow liquid
Calibrator 2	1 × 0.5 ml	human serum containing ft3 in concentration approx. 4.5 pg/ml; pale yellow liquid
Calibrator 3	1 × 0.5 ml	human serum containing ft3 in concentration approx. 10.0 pg/ml; pale yellow liquid
Calibrator 4	1 × 0.5 ml	human serum containing ft3 in concentration approx. 20.0 pg/ml; pale yellow liquid
Control serum	1 × 0.5 ml	human serum based control containing ft3; colourless or pale yellow liquid
Washing solution (concentrated 25-fold)	1 × 50 ml	phosphate saline buffer; colourless or pale yellow liquid
TMB/substrate solution	1 × 12 ml	ready to use; citric acid buffer containing TMB and H ₂ O ₂ ; colourless liquid
Stopping reagent 0.2M H ₂ SO ₄	1 × 25 ml	ready to use; 0.20 mol/l sulphuric acid solution; colourless liquid
Protective film	1	
Plastic dish	2	
Plastic zip-lock bag	1	

Exact concentration levels for calibrators and control serum are given on the labels and certificates of analysis on a lot specific basis. For SI units: pg/ml x 1.536 = pmol/l.

All components are stable until expiration date of the kit when stored at 2–8 °C in a tightly sealed package. Expiration date is indicated on the package.

Once opened, the components should be used within 2 months. Concentration of preserving agents: <=0.1 %.

Materials and equipment required but not provided

- purified water
- automatic or semiautomatic, adjustable or preset pipettes or multipipettes
- disposable pipette tips
- microplate shaker
- automatic microplate washer
- microplate reader equipped with 450 nm filter

Safety notes

- human origin material used in the preparation of the calibrators and control serum has been tested and found non reactive for hepatitis B surface antigen (HBsAg), antigen p24 HIV-1, antibodies to hepatitis C virus and antibodies to human immunodeficiency virus (HIV-1 and HIV-2)
- as no known test method can offer complete assurance that infectious agents are absent, reagents and samples should be handled as if capable of transmitting infectious disease; any equipment directly in contact with samples and reagents should be considered as contaminated
- do not eat, drink, smoke or apply cosmetics in the laboratory
- do not pipette by mouth
- avoid any contact of the reagents and samples with the skin and mucosa; wear lab coats and disposable gloves when handling them; thoroughly wash your hands after work
- avoid spilling samples or solutions containing samples. Wipe spills immediately and decontaminate affected surfaces
- all materials contacted with specimens or reagents, including liquid and solid waste, should be inactivated by validated procedures (autoclaving or chemical treatment) and disposed in accordance with applicable local law regulations

Precautions

- do not use reagents without label or with damaged label/package
- do not use expired reagents
- do not change the assay procedure; perform all subsequent steps without interruption
- do not mix reagents from different lots
- do not mix the caps of vials
- do not run the EIA test in the presence of reactive vapours (acid, alkaline, aldehyde), dust or metals
- do not let the wells dry once the assay has been started
- do not use the same container and tips for different liquid components of the kit and samples
- do not reuse the coated plates
- do not reuse the removed protective film
- do not expose the reagents to excessive heat or sunlight during storage and test procedure
- do not freeze the reagents

Collection and handling of specimens

- collect blood specimens according to the current practices
- use serum for testing; performances of the test have not been evaluated on other biological fluids
- separate the clot or red cells from serum as soon as possible to avoid any haemolysis
- do not use sera preserved with sodium azide
- do not use contaminated, hyperlipaemic and hyperhaemolysed specimens
- the samples with hyperproteinaemia and hyperbilirubinaemia were not specially tested
- before testing samples with observable particulate matter should be clarified by centrifugation
- suspended fibrin particles or aggregates may yield reactive results
- do not heat the samples
- samples can be stored at 2–8 °C within 72 hours or deep-frozen at -20 °C
- no more than one freeze/thaw cycle is allowed

Procedural notes

- before use wait 30 minutes for the reagents to stabilize to room temperature (20–25 °C)
- check appearance of the reagents
- lost vacuum in the bag of the coated plate will not affect the performance of the test
- check the pipettes and other equipment for accuracy and correct operation
- the washing procedure is a critical step; for the detailed washer settings see section “Washing procedure”
- for the description of test procedure with the automated analyzers see section “Automated analyzers”

Washing procedure

Please contact your representative for protocols for recommended washers and procedures. In general the following protocol is recommended:

- flow-through washing with a volume not less than 300 µl per well is used
- repeat 5 times
- do not allow the wells to become dry during the assay procedure
- ensure that no liquid is left in the well (use double aspiration in the final step where possible)
- avoid to tap out the plate
- residual volume lower than 10 µl is not critical for following steps of the test procedure
- when using a microplate washer clean the wash head frequently to prevent contamination

Preparation of reagents

Number of strips to be used	1	2	3	4	5	6	7	8	9	10	11	12
Working washing solution: mix the reagents thoroughly by inversion												
Stability: 14 days at 18–24 °C or 28 days at 2–8 °C												
Washing solution (concentrated 25-fold), ml	3.0	6.0	9.0	12.0	15.0	18.0	21.0	24.0	27.0	30.0	33.0	40.0
Purified water, ml	72.0	144.0	216.0	288.0	360.0	432.0	504.0	576.0	648.0	720.0	792.0	960.0

Test procedure

abia ft3 for the quantitative determination of free triiodothyronine (fT3) concentration in human serum

- 1 Take the required number of coated strips. Place the unused strips back into the bag; reseal the foil-lined package in plastic zip-lock bag. Do not remove desiccant.
 - 2 Analyse each calibrator, control serum, and sample duplicate.
Add 25 µl of calibrators 0 - 4 into appropriate wells.
Add 25 µl of control serum into appropriate wells.
Add 25 µl of samples to be tested in rest of the wells.
The total time should not exceed 10 min.
 - 3 Add 100 µl conjugate into each well. Cover the plate with protective film.
 - 4 Incubate in microplate shaker (approximately 500-800 rpm) for 60 minutes at room temperature 20–25 °C.
 - 5 Remove the protective film slowly and carefully to prevent splashes. Aspirate the contents of all wells into a container for biohazardous waste (containing disinfectant).
Add not less than 300 µl of working washing solution into each well and aspirate. Perform this procedure 5 times. Use double aspiration in the final step where possible.
 - 6 Add 100 µl of TMB/substrate solution to all the wells. Keep the plates in a dark place for 25 ± 5 minutes at 20–25 °C.
 - 7 Add 150 µl of stopping reagent into each well. Mix gently for 5–10 sec.
 - 8 Read the optical density at 450 nm using a plate reader within 20 minutes after stopping reaction.
-

Automated analyzers

Validated protocols for automated analyzers can be obtained from your representative. For the instrumentation without established validated protocol follow section “Test procedure” and ensure all requirements described in section “Precautions” are followed. All protocols for automated analyzers must be fully validated prior usage.

Calculation and interpretation of the results

Assay validation

Results of an assay are valid if the following criteria for the controls are met.

The absorbance (OD) of control serum should be within established range.
The absorbance (OD) of calibrator 0 should be greater than 1.300.

Calculation procedure

- 1 Calculate the mean optical density of each calibrator duplicate.
- 2 Calculate the mean optical density of each sample duplicate.
- 3 Draw a calibration curve on linear graph paper with the mean optical densities on the Y-axis and the calibrator concentrations on the X-axis.
- 4 Read the values of the unknowns directly off the calibration curve.
If immunoassay software is being used, a 4-parameter curve is recommended.

Example	OD 1	OD 2	Mean OD	Value, pg/ml
Calibrator 0	2.624	2.578	2.601	0.00
Calibrator 1	1.985	1.976	1.981	1.50
Calibrator 2	1.397	1.423	1.410	4.50
Calibrator 3	0.889	0.905	0.897	10.00
Calibrator 4	0.574	0.594	0.584	20.00
Sample	1.690	1.712	1.701	2.60

This data is for illustration only and should **not be used** to calculate of samples. Each user should obtain his or her own data and standard curve.

Performance characteristics

Analytical sensitivity

The analytical sensitivity (limit of detection) was calculated by determining the variability of the calibrator 0 based on 27 replicate analyses less $2 \times$ SD. Limit of detection defined at 0.25 pg/ml.

Specificity	Concentration, $\mu\text{g/ml}$	Cross reactivity, %
L-thyroxine (T4)	2.50	5.2E-06
Diiodothyronine (T2)	0.25	3.5E-05
Tetraiodothyroacetat (T4A)	10.00	1.6E-06

Precision	Mean value, pg/ml	SD	CV, %
Intra-assay, sample 1	2.34	0.102	4.30
Intra-assay, sample 2	6.09	0.135	2.20
Inter-assay, sample 1	2.30	0.118	5.10
Inter-assay, sample 2	5.97	0.217	3.60

Accuracy

The assay was compared with a chemiluminescent microparticle immunoassay as a reference test. The total number of specimens was 726. The values ranged from 1.23 to 33.27 pg/ml. The least square regression equation and the correlation coefficient were computed for abia fT3 in comparison with the reference method.

The least square regression analysis was $y = 1.51(x) - 1.96$ with correlation coefficient of 0.93.

Expected normal value

	Range, pg/ml	
Adult population	1.20	4.20

Normal value ranges may vary slightly among different laboratories. It is strongly recommended that each laboratory should determine its own range of expected normal values.

Limitations of test

- the assay was validated only for the determination of T3 (triiodothyronine) in human serum
- the results obtained with this assay should never be used as the sole basis for clinical diagnosis. Any laboratory result is only a part of the total clinical picture of the patient
- serum T3 free values may be changed during pregnancy
- circulating antibodies to T3 and hormone-binding inhibitors may interfere in the performance of the assay
- a decrease in free triiodothyronine values is found with protein wasting diseases, certain liver diseases and administration of diphenylhydantoin or salicylates
- in rare conditions associated with extreme variations in albumin binding capacity for T3 – such as familial dysalbuminemic hyperthyroxinemia – direct assessment of free T3 may be misleading
- performance of this test has not been established with neonatal specimens

References

1. Lundberg P.R., Clin. Chem., Vol. 28, 1241 (1982).
2. Wild D, Immunoassay Handbook, Stockton Press, 339 (1994).
3. Ekins, "Free hormon assay". Nuclear Medicine Communications, 14, 676-688 (1993).

Key to symbols used



Manufacturer



For in vitro diagnostic use



Catalogue number



Batch code



Expiry date



Storage temperature limitation



Do not use if package is damaged



Do not reuse



Sufficient for [n] tests



Consult Instructions for use



Caution, consult documents



Changes highlighted

Hazard and precautionary statements for certain kit components

Stopping reagent



Warning

H315

Causes skin irritation.

H319

Causes serious eye irritation.

P264

Wash hands thoroughly after handling.

P280

Wear protective gloves/protective clothing/eye protection/face protection.

P302 + P352

IF ON SKIN: Wash with plenty of soap and water.

P305 + P351 +
P338

IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.

Conjugate, calibrators 0 - 4, control serum



Warning

H317

May cause an allergic skin reaction.

P261

Avoid breathing dust/fume/gas/mist/vapours/spray.

P280

Wear protective gloves/protective clothing/eye protection/face protection.

P302 + P352

IF ON SKIN: Wash with plenty of soap and water.

P333 + P313

If skin irritation or rash occurs: Get medical advice/attention.

Attention!

For complete precautionary statements and detailed information see safety data sheets (SDS).



AB Diagnostic Systems GmbH
Sportfliegerstraße 4
12487 Berlin
Germany

☎ +49 30 208 987 160
☎ +49 30 208 987 199
✉ info@ab-ds.de
www.ab-ds.de

