

abia T4 total




REF DK.035.01.3

IVD



Note: Changes highlighted ★

abia

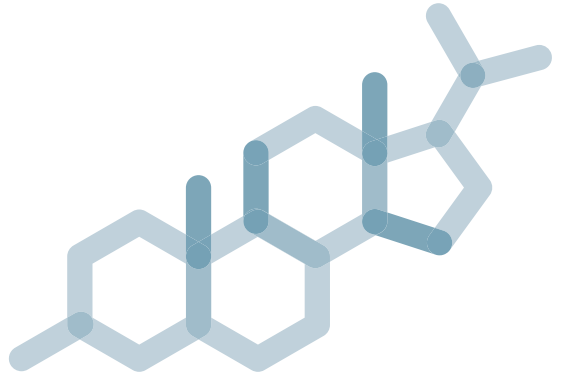

Intended use

Abia T4 total enzyme immunoassay for the quantitative determination of total thyroxine (T4) concentration in human serum.

The assay is intended for aid in the assessment of thyroid status and diagnosis of thyroid disease. For professional use only.

Clinical value

Thyroxine, the principal thyroid hormone, circulates in blood almost completely bound to carrier proteins.

The main carriers are thyroxine-binding globulin (TBG) with 70%, thyroxine binding pre-albumin (TBPA) with 20% and albumin with 10%. However, only the free (unbound) portion of thyroxine is responsible for the biological action. Further, the concentrations of the carrier proteins are altered in many clinical conditions, such as pregnancy.

In normal thyroid function as the concentrations of the carrier proteins alters, the total thyroxine level changes so that the free thyroxine concentration remains constant. Diseases affecting thyroid function may present a wide array of confusing symptoms.

Measurement of total T4 by immunoassay is the most reliable and convenient screening test available to determine the presence of thyroid disorders in patients. Increased levels of T4 have been found in hyper-thyroidism due to Grave's disease and Plummer's disease and in acute and subacute thyroiditis. Low levels of T4 have been associated with congenital hypothyroidism, myxedema, chronic thyroiditis (Hashimoto's disease), and with some genetic abnormalities.

Principle of the test

Abia T4 total is a one-step immunoassay, based on the principle of the competitive method.

Thyroxine present in the sample and the labeled enzyme-thyroxine in the conjugate compete for binding to the capture antibody on the anti-T4 coated microplate. The enzyme activity in the antibody-bound fraction is inversely proportional to the native thyroxine concentration.

The unbound components are removed by washing. After addition of the solution containing TMB and hydrogen peroxide, the wells with bound conjugate develop a blue colour which is converted to yellow after the reaction has been stopped with sulphuric acid.

The colour intensity is inversely proportional to the concentration of the native thyroxine in the specimen and can be read at 450 nm.

Kit contents

	S	
T4 Ab coated plate	1	polystyrene plate 12 × breakable 8-well strips coated with monoclonal anti-thyroxine Ab
Conjugate	1 × 12 ml	HRP-labeled thyroxine; transparent or slightly opalescent pink liquid
T4 buffer ANS	1 × 12 ml	binding protein inhibitors buffer; transparent olive-brown liquid
Calibrator 0	1 × 0.5 ml	human serum not containing T4; pale yellow liquid
Calibrator 1	1 × 0.5 ml	human serum containing T4 in concentration approx. 10 nmol/l; pale yellow liquid
Calibrator 2	1 × 0.5 ml	human serum containing T4 in concentration approx. 50 nmol/l; pale yellow liquid
Calibrator 3	1 × 0.5 ml	human serum containing T4 in concentration approx. 100 nmol/l; pale yellow liquid
Calibrator 4	1 × 0.5 ml	human serum containing T4 in concentration approx. 200 nmol/l; pale yellow liquid
Calibrator 5	1 × 0.5 ml	human serum containing T4 in concentration approx. 400 nmol/l; pale yellow liquid
Control serum	1 × 0.5 ml	human serum based control containing T4; colourless or pale yellow liquid
Washing solution (concentrated 25-fold)	1 × 50 ml	phosphate saline buffer; colourless or pale yellow liquid
TMB/substrate solution	1 × 12 ml	ready to use; citric acid buffer containing TMB and H ₂ O ₂ ; colourless liquid
Stopping reagent 0.2M H ₂ SO ₄	1 × 25 ml	ready to use; 0.20 mol/l sulphuric acid solution; colourless liquid
Protective film	1	
Plastic dish	2	
Plastic zip-lock bag	1	

Exact concentration levels for calibrators and control serum are given on the labels and certificates of analysis on a lot specific basis. For conventional units: nmol/l x 0.078 = µg/dl.

All components are stable until expiration date of the kit when stored at 2–8 °C in a tightly sealed package. Expiration date is indicated on the package.

Once opened, the components should be used within 2 months. Concentration of preserving agents: <=0.1 %.

Materials and equipment required but not provided

- purified water
- automatic or semiautomatic, adjustable or preset pipettes or multipipettes
- disposable pipette tips
- automatic microplate washer
- microplate reader equipped with 450 nm filter

Safety notes

- human origin material used in the preparation of the calibrators and control serum has been tested and found non reactive for hepatitis B surface antigen (HBsAg), antigen p24 HIV-1, antibodies to hepatitis C virus and antibodies to human immunodeficiency virus (HIV-1 and HIV-2)
- as no known test method can offer complete assurance that infectious agents are absent, reagents and samples should be handled as if capable of transmitting infectious disease; any equipment directly in contact with samples and reagents should be considered as contaminated
- do not eat, drink, smoke or apply cosmetics in the laboratory
- do not pipette by mouth
- avoid any contact of the reagents and samples with the skin and mucosa; wear lab coats and disposable gloves when handling them; thoroughly wash your hands after work
- avoid spilling samples or solutions containing samples. Wipe spills immediately and decontaminate affected surfaces
- all materials contacted with specimens or reagents, including liquid and solid waste, should be inactivated by validated procedures (autoclaving or chemical treatment) and disposed in accordance with applicable local law regulations

Precautions

- do not use reagents without label or with damaged label/package
- do not use expired reagents
- do not change the assay procedure; perform all subsequent steps without interruption
- do not mix reagents from different lots
- do not mix the caps of vials
- do not run the EIA test in the presence of reactive vapours (acid, alkaline, aldehyde), dust or metals
- do not let the wells dry once the assay has been started
- do not use the same container and tips for different liquid components of the kit and samples
- do not reuse the coated plates
- do not reuse the removed protective film
- do not expose the reagents to excessive heat or sunlight during storage and test procedure
- do not freeze the reagents

Collection and handling of specimens

- collect blood specimens according to the current practices
- use serum for testing; performances of the test have not been evaluated on other biological fluids
- separate the clot or red cells from serum as soon as possible to avoid any haemolysis
- do not use sera preserved with sodium azide, thiomersal, phenol
- do not use contaminated, hyperlipaemic and hyperhaemolysed specimens
- the samples with hyperproteinaemia and hyperbilirubinaemia were not specially tested
- before testing samples with observable particulate matter should be clarified by centrifugation
- suspended fibrin particles or aggregates may yield reactive results
- do not heat the samples
- samples can be stored at 2–8 °C within 72 hours or deep-frozen at -20 °C
- no more than one freeze/thaw cycle is allowed

Procedural notes

- before use wait 30 minutes for the reagents to stabilize to room temperature (20–25 °C)
- check appearance of the reagents
- lost vacuum in the bag of the coated plate will not affect the performance of the test
- check the pipettes and other equipment for accuracy and correct operation
- the washing procedure is a critical step; for the detailed washer settings see section “Washing procedure”
- for the description of test procedure with the automated analyzers see section “Automated analyzers”

Washing procedure

Please contact your representative for protocols for recommended washers and procedures. In general the following protocol is recommended:

- flow-through washing with a volume not less than 300 µl per well is used
- repeat 5 times
- do not allow the wells to become dry during the assay procedure
- ensure that no liquid is left in the well (use double aspiration in the final step where possible)
- avoid to tap out the plate
- residual volume lower than 10 µl is not critical for following steps of the test procedure
- when using a microplate washer clean the wash head frequently to prevent contamination

Preparation of reagents

Number of strips to be used	1	2	3	4	5	6	7	8	9	10	11	12
Working conjugate solution: mix the reagents thoroughly by inversion Stability: do not store, only prepare for immediate use												
Conjugate, ml	1.0	2.0	3.0	4.0	5.0	6.0	7.0	8.0	9.0	10.0	11.0	12.0
T4 buffer ANS, ml	1.0	2.0	3.0	4.0	5.0	6.0	7.0	8.0	9.0	10.0	11.0	12.0
Working washing solution: mix the reagents thoroughly by inversion Stability: 14 days at 18–24 °C or 28 days at 2–8 °C												
Washing solution (concentrated 25-fold), ml	3.0	6.0	9.0	12.0	15.0	18.0	21.0	24.0	27.0	30.0	33.0	40.0
Purified water, ml	72.0	144.0	216.0	288.0	360.0	432.0	504.0	576.0	648.0	720.0	792.0	960.0

Test procedure

abia T4 total for the quantitative determination of total thyroxine (T4) concentration in human serum

- 1 Take the required number of coated strips. Place the unused strips back into the bag; reseal the foil-lined package in plastic zip-lock bag. Do not remove desiccant.

- 2 Analyse each calibrator, control serum, and sample duplicate.
Add 25 µl of calibrators 0 - 5 into appropriate wells.
Add 25 µl of control serum into appropriate wells.
Add 25 µl of samples to be tested in rest of the wells.
The total time should not exceed 10 min.

- 3 Add 200 µl conjugate working solution into each well.
Mix the contents of the wells for 30 seconds by careful tapping on the edge of the plate, then cover the plate with protective film.

- 4 Incubate for 90 minutes at room temperature 20–25 °C.

- 5 Remove the protective film slowly and carefully to prevent splashes. Aspirate the contents of all wells into a container for biohazardous waste (containing disinfectant).
Add not less than 300 µl of working washing solution into each well and aspirate. Perform this procedure 5 times. Use double aspiration in the final step where possible.

- 6 Add 100 µl of TMB/substrate solution to all the wells. Keep the plates in a dark place for 15–20 minutes at 20–25 °C.

- 7 Add 150 µl of stopping reagent into each well. Mix gently for 5–10 sec.

- 8 Read the optical density at 450 nm using a plate reader within 20 minutes after stopping reaction.

Automated analyzers

Validated protocols for automated analyzers can be obtained from your representative. For the instrumentation without established validated protocol follow section “Test procedure” and ensure all requirements described in section “Precautions” are followed. All protocols for automated analyzers must be fully validated prior usage.

Calculation and interpretation of the results

Assay validation

Results of an assay are valid if the following criteria for the controls are met.

The absorbance (OD) of control serum should be within established range.
The absorbance (OD) of calibrator 0 should be greater than 1.300.

Calculation procedure

- 1 Calculate the mean optical density of each calibrator duplicate.
- 2 Calculate the mean optical density of each sample duplicate.
- 3 Draw a calibration curve on linear graph paper with the mean optical densities on the Y-axis and the calibrator concentrations on the X-axis.
- 4 Read the values of the unknowns directly off the calibration curve.
If immunoassay software is being used, a 4-parameter curve is recommended.

Example	OD 1	OD 2	Mean OD	Value, nmol/l
Calibrator 0	3.138	3.092	3.115	0.00
Calibrator 1	2.089	2.134	2.112	11.00
Calibrator 2	0.969	0.990	0.980	51.00
Calibrator 3	0.587	0.603	0.595	94.00
Calibrator 4	0.323	0.327	0.325	190.00
Calibrator 5	0.182	0.185	0.184	400.00
Sample	0.582	0.707	0.645	88.80

This data is for illustration only and should **not be used** to calculate of samples. Each user should obtain his or her own data and standard curve.

Performance characteristics

Analytical sensitivity

The analytical sensitivity (limit of detection) was established according to CLSI EP-17A2 protocol. Limit of detection defined at 5.00 nmol/l.

Specificity	Concentration, µg/ml	Cross reactivity, %
Triiodothyronine (T3)	1.00	0.71
Diiodothyronine (T2)	200.00	0.004
Tetraiodothyroacetat (T4A)	1.00	0.75

Precision	Mean value, nmol/l	SD	CV, %
Intra-assay, sample 1	73.30	3.30	4.40
Intra-assay, sample 2	144.10	7.90	5.50
Intra-assay, sample 3	263.90	10.80	4.10
Inter-assay, sample 1	73.30	4.00	5.50
Inter-assay, sample 2	144.1	10.50	7.30
Inter-assay, sample 3	263.90	18.90	7.20

Accuracy

The assay was compared with a chemiluminescent microparticle immunoassay as a reference test. The total number of specimens was 336. The values ranged from 9.70 to 311.50 nmol/l. The least square regression equation and the correlation coefficient were computed for abia T4 total in comparison with the reference method.

The least square regression analysis was $y = 0.996(x) + 4.89$ with correlation coefficient of 0.95.

Expected normal value

	Range, nmol/l	
Adult population	59.00	153.0

Normal value ranges may vary slightly among different laboratories. It is strongly recommended that each laboratory should determine its own range of expected normal values.













Limitations of test

- the assay was validated only for the determination of T4 (thyroxine) in human serum
- the results obtained with this assay should never be used as the sole basis for clinical diagnosis. Any laboratory result is only a part of the total clinical picture of the patient
- serum T4 total values may be changed during pregnancy
- circulating antibodies to T4 and hormone-binding inhibitors may interfere in the performance of the assay
- a decrease in total thyroxine values is found with protein wasting diseases, certain liver diseases and administration of testosterone, diphenylhydantoin or salicylates
- in rare conditions associated with extreme variations in albumin binding capacity for T4 – such as familial dysalbuminemic hyperthyroxinemia – direct assessment of T4 may be misleading

References

1. Sterling L. Diagnosis and treatment of Thyroid Disease. CRC Press; 19-51 (1975).
2. Nelson J.C., Wilcox R.B. Analytical performance of free and total thyroxine assays. Clinical Chemistry; 42:1, 146-154 (1996).

Key to symbols used

	Manufacturer
	For in vitro diagnostic use
	Catalogue number
	Batch code
 YYYY-MM-DD	Expiry date
 2°C 8°C	Storage temperature limitation
	Do not use if package is damaged
	Do not reuse
 Σ_n	Sufficient for [n] tests
	Consult Instructions for use
	Caution, consult documents
	Changes highlighted

Hazard and precautionary statements for certain kit components

Stopping reagent



Warning

H315	Causes skin irritation.
H319	Causes serious eye irritation.
P264	Wash hands thoroughly after handling.
P280	Wear protective gloves/protective clothing/eye protection/face protection.
P302 + P352	IF ON SKIN: Wash with plenty of soap and water.
P305 + P351 + P338	IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.

Conjugate, T4 buffer ANS, calibrators 0 - 5, control serum



Warning

H317	May cause an allergic skin reaction.
P261	Avoid breathing dust/fume/gas/mist/vapours/spray.
P280	Wear protective gloves/protective clothing/eye protection/face protection.
P302 + P352	IF ON SKIN: Wash with plenty of soap and water.
P333 + P313	If skin irritation or rash occurs: Get medical advice/attention.

Attention!

For complete precautionary statements and detailed information see safety data sheets (SDS).



AB Diagnostic Systems GmbH
Sportfliegerstraße 4
12487 Berlin
Germany

☎ +49 30 208 987 160
☎ +49 30 208 987 199
✉ info@ab-ds.de
www.ab-ds.de

